

LESS IS MORE...

EFFICIENT & POWERFUL SCREENER

Proven Signal Quality

Based on SOMNOtouch™ RESP - with flow/CPAP pressure/snore, SpO₂, pulse rate, plethysmogram, activity, effort, position and patient marker

Easy Handling

Easy to apply, pre-programmed or manual start which can run for up to 18 h

Simple to Use

Pre-loaded montage and sleep report. Software with powerful tools for fast manual scoring

Outstanding Cost/Benefit Ratio

Be competitive whilst utilising the best respiratory sleep screener device - from the thought leaders in sleep diagnostics

Small Compact Design

Same footprint as a credit card, with built-in Li-Ion battery, allowing unparalleled comfort for the patient and ease of use for the clinic



RECURSOS EN
 INSTRUMENTACIÓN
 CLÍNICA S.A. DE C.V.

The **SOMNOtouch™ RESP eco*** – joins the SOMNOtouch™ family of products and is positioned primarily at the physician who only requires a Level III device.

Responding to the growing demand for low cost home sleep apnea testing, the SOMNOtouch™ RESP eco embodies the term “less is more” – with 11 channels including one optional sensor: abdomen effort. Using intelligent connect™ and a combined data and charging USB cable, it is exceptionally easy to set up and use.

*FDA approved for adults only


STAY CURRENT WITH FREE AUTOMATIC SOFTWARE UPDATES

Optimize your sleep screening with our SOMNOtouch™ RESP eco

- ◆ Correlation between body position and respiratory events – to better differentiate between patients requiring positional training devices or CPAP therapy
- ◆ Cheyne Stokes analysis in combination with pulse rate, gives insight to cardiorespiratory health
- ◆ Computer aided arousal detection on the plethysmogram enables you to score RERAs and define sleep fragmentation
- ◆ Distinguish between AHI and RDI using the RERAs
- ◆ Extensive CPAP pressure report – define the ideal pressure for your patients

Simple easy to use interface

- ◆ Easy to use for both physician and patient
- ◆ Quick start function – one standard montage
- ◆ Pre-configured report for helpful data processing
- ◆ Marker button to notify interesting events

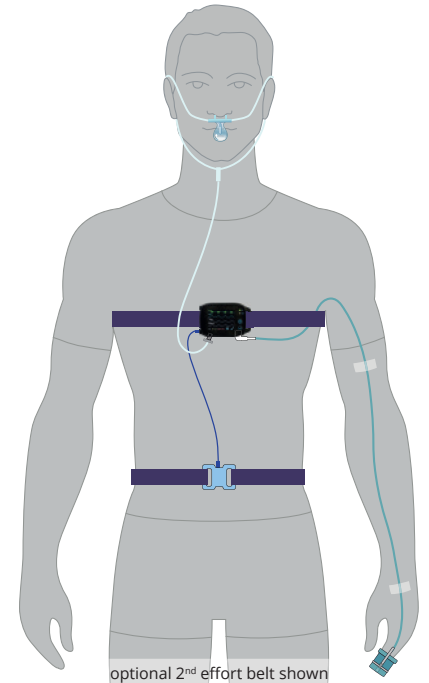


No thermistor needed

Measure mouth breathers with a nasal-oral cannula. Then process the signal with our linearization algorithm for results that have the same sensitivity and specificity as a traditional thermistor¹.

¹Diagnostic utility of a nasal-oral cannula with linearized pressure flow in comparison to AASM recommended combination of thermal and nasal pressure sensor.


Küchler, G. et al., Eur Respir J 09.2017, 50 (suppl 61) PA2297; DOI: 10.1183/1393003.congress-2017.PA2297.

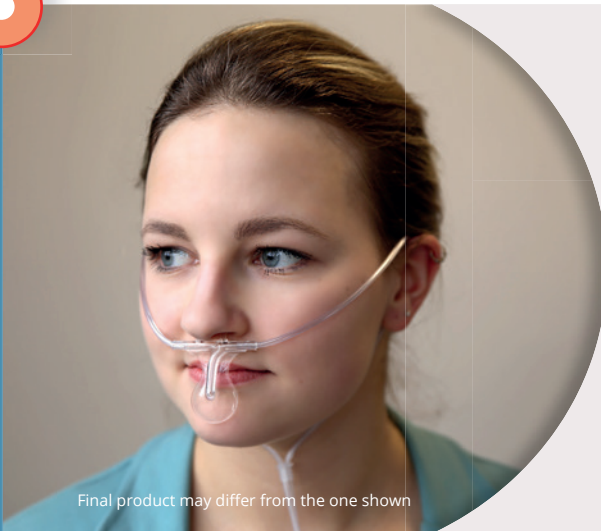

Device & analysis software

- ◆ 50 min fast charge for an 8 h night recording
- ◆ Quick data transfer (Approx. 90 s for a full night's study)
- ◆ PC interface with graphic-based control
- ◆ Powerful DOMINO light software
- ◆ Manual & computer aided scoring available

Respiratory Analysis		REM	Non-REM	Sleep
Obstructive	194 (20.1)	-	-	-
Mixed	89 (13.3)	-	-	-
Central	93 (13.9)	-	-	316 (47.3)
Under A	-	-	-	117 (17.5)
Total Apn	310 (47.3)	-	-	64.8
Hypnoea	117 (17.5)	-	-	-
AHI	433 (64.8)	-	-	-
Limitations	-	-	-	-
RDI	-	-	-	-

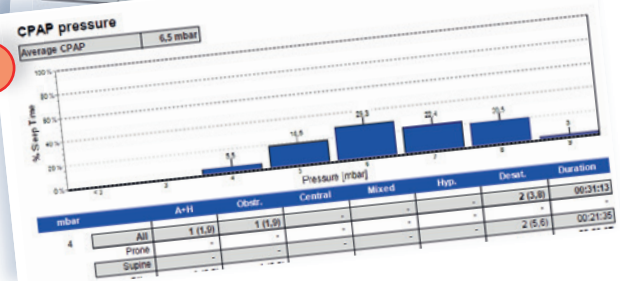

Excerpt from the pre-configured report